

TRIPULSAR 9 by Altered States Limited

The unit is based on a microprocessor controlled system which allows for multi function use, precise timing, and efficiency

It is compact with digital and multi coloured LED.s which are easy to use and care for.

The Tripulsar 9 is a multi function unit that combines;

- Magnetic Pulsar .MP.
- Bob Beck Zapper .Z.
- Colloidal Silver Generator .CS.

OPERATION

- To Turn on press ON-Off button and release. Once system is powered up it will go to the Default Zapper mode
- Zapper at lowest output level and 5 minute timer
- Press .Function. button to required function Zapper C-Silver or Magnetic Pulsar
- To select the INTENSITY when using the
- Use the .TIMER. button to select desired time.
- For Zapper and C-Silver it is 5 to 120 minutes.
- Pulsar is 5-20 minutes
- Press .START. button to start or Pause the program
- Pressing the .ON-OFF. button will stop the program at any time during use. It can also be used to cancel the current timer.

WARNING

➤ The TRIPULSAR 9 has a **very high voltage** and a **very strong magnetic field** output. Care must be taken while using the unit.

➤ There must be **NO** steel parts around during use. Metal objects will interfere with the magnetic pulses.

➤ Anyone who has a Pacemaker or similar should **NOT** use this machine

The Magnetic Pulsar has a high power usage and will generate a large amount of heat.

To avoid potential damage to the unit do not operate for any longer than 20 minutes

Leave at least half an hour between each session

➤ The Tripulsar 9 must be kept dry and away from moisture and high humidity. It is advised that children should NOT operate this device.

➤ As the unit could overheat ENSURE that there is nothing covering it during operation

➤ If the machine overheats, begins to smell or has a broken case it must be turned off immediately and not used until repaired.

➤ Service and Repair must be done by a qualified electrical service technician or authorized service agency.

➤ **Contact Altered States Limited immediately if your device appears faulty.**

FUNCTIONS

Beck Zapper/Colloidal Silver Generator/Magnetic Pulser

Z = Zapper

CS = Colloidal Silver

MP = Magnetic Pulser

This information here is based on Dr. Bob Becks. original protocol for using the blood electrifier and colloidal silver generator.

According to his research, he found a way to kill all known viruses with a four pronged treatment: 1) Ozonated water 2) Colloidal silver water 3) blood purifier (zapping device) 4) Magnetic pulsar.

This unit is made to specifications designed by Dr. Bob Beck. It can be used in protocols #2 & #3 as listed above. As all people are different, results may vary. These units are most effective when used according to Dr. Bob Becks. protocol. Nothing is guaranteed. Put simply, the closer you match Becks protocol, the better results you may achieve.

Research from Harvard, MIT and Albert Einstein College of Medicine has shown that micro currents are known to eliminate viruses, parasites, fungi, bacteria and pathogens in the blood. This unit emits those same micro currents.

It has been a long known fact, that silver colloids greatly assist in eliminating known pathogens and prevents opportunistic infections.

Making Colloidal Silver Water

Colloidal Silver water is very susceptible to light and temperature change so it must be kept in dark amber bottles or opaque containers. A stable room temperature environment is ideal.

The silver rods supplied are 99.99% pure silver. A higher grade of silver of 99.999% purity can be used Lower grade silver or sterling silver will contain nickel which is **toxic and must not** be used.

[How to use Colloidal Silver in the Bob Beck protocol](#)

Select .CS..

- Select the Yellow led by pushing the on off button then the Function Button
- The yellow LED will light up
- Connect the silver rods to the alligator clips; plug this lead to the .output. socket on the main device. Place the silver rods over the top lip of the glass (see fig. 1).
- Place the silver rods 4-5cm apart. Keep them parallel and do not let them touch (otherwise it is likely to .short. the unit out and render it ineffective).
-
- fig. 1
- Use 250ml distilled water.
- Distilled water is non-conductive, so it is necessary to create conductivity in the water This can be obtained by either placing, two to three drops of lemon juice or raising the water temperature to .luke-warm. often One rod will emit bubbles, the other, a grey mist.
- Generate for 5-15 minutes.
- [Article #3:How to use Colloidal Silver in the Bob Beck protocol](#)
- **Push Start**

Zapping

Before zapping, it is very important to eliminate **ALL** herbs (including garlic), dietary supplements, alcohol, recreational drugs and medications. Stop taking these at least **24 hours** prior to using the zapper

(preferably 4-7 days before zapping). You may then take medicine or vitamins straight AFTER zapping. This is because zapping can allow medicines, drugs and herbs to enter the body's cells and it can actually

magnify their effect 20-30 times so while you are zapping with these in your body, the supplements are amplified dramatically.

➤ Zapping times can vary between 15 minutes a day to 2 hours a day.

➤ It is very important to drink at least 3-4 glasses of filtered or purified water (even distilled water) during the zapping process. This will help to flush your system and allow detoxification to occur. **YOU MUST DRINK PLENTY OF WATER WHILE ZAPPING** or you will not detoxify your body correctly.

If you feel unwell after zapping reduce the zapping time. The unwell feeling is the body detoxifying. This is a good sign but it is not necessary to feel unwell every time you zap.

Select .Z.

➤ Insert the silver electrodes into the cotton sleeves.

➤ Mix up a small amount of purified water with sea salt and wet the cotton sleeves with this solution. This is a saline solution which will aid with conductivity between the electrodes and your skin.

➤ **DO NOT PLACE** the electrodes on bare skin as this may burn or give an uncomfortable feeling to the skin.

➤ Turn Machine on

➤ Select the Green led by pushing the on off button then the Function Button

➤ The Green LED will light up

➤ Choose Function Z for Zapper

➤

➤

It is important to place the electrodes correctly otherwise zapping will not be effective.

➤

➤ Set Intensity to the first green LED,,, (this can be altered to suit while the unit is running)

➤ Set Time (see link below)

➤ [Article #1:How to use Blood Purifier or Blood Electrification](#)

➤ **Press Start**

Magnetic PULSAR

➤ Turn Unit on

➤ Using the Function button choose .MP.

➤ Set Time 20min max

➤ Place north **.N.** or its opposite **.S.** on the desired area.

➤ See here for more info

<http://alteredstates.net/barry/rifeCD/Library/northsouth%20facing%20magnetic%20fields.pdf>

➤

➤ [Article #2:How to use Pulsed Kilogauss Magnetic Fields \(i.e. Magnetic Pulser\)](#)

➤

➤ Run for twenty minutes two to three times daily or as required

Article #2:How to use Pulsed Kilogauss Magnetic Fields (i.e. Magnetic Pulser)


WARNING



- The TRIPULSAR 9 has a **very high voltage** and a **very strong magnetic field** output. Care must be taken while using the unit.
- There must be **NO** steel parts around during use. Metal objects will interfere with the magnetic pulses.
- Anyone who has a Pacemaker or similar should **NOT** use this machine
- The Tripulsar 9 must be kept dry and away from moisture and high humidity. It is advised that children should NOT operate this device.
- As the unit could overheat ENSURE that there is nothing covering it during operation
- If the machine overheats, begins to smell or has a broken case it must be turned off immediately and not used until repaired.
- Service and Repair must be done by a qualified electrical service technician or authorized service agency.
- **Contact Altered States Limited immediately if your device appears faulty.**

Disclaimer

This material is being offered as theoretical/experimental information only. No guarantees are offered or implied as to the safety or efficiency of the product. This information is not intended to replace medical advice offered by physicians. For medical advice in dealing with health challenges, please consult with your health care professional. Altered States, including management and staff disclaim liability for any loss, arising directly or indirectly from the use of the above information.

Magnetic Pulsar Combo

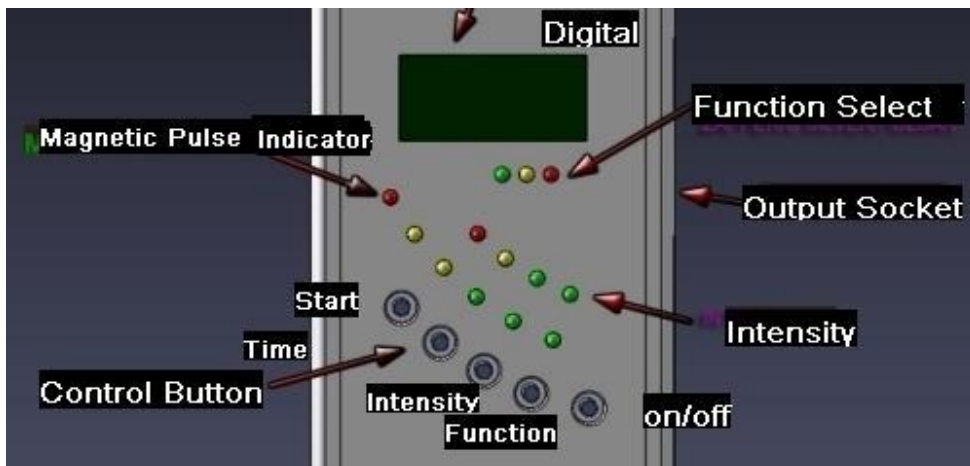

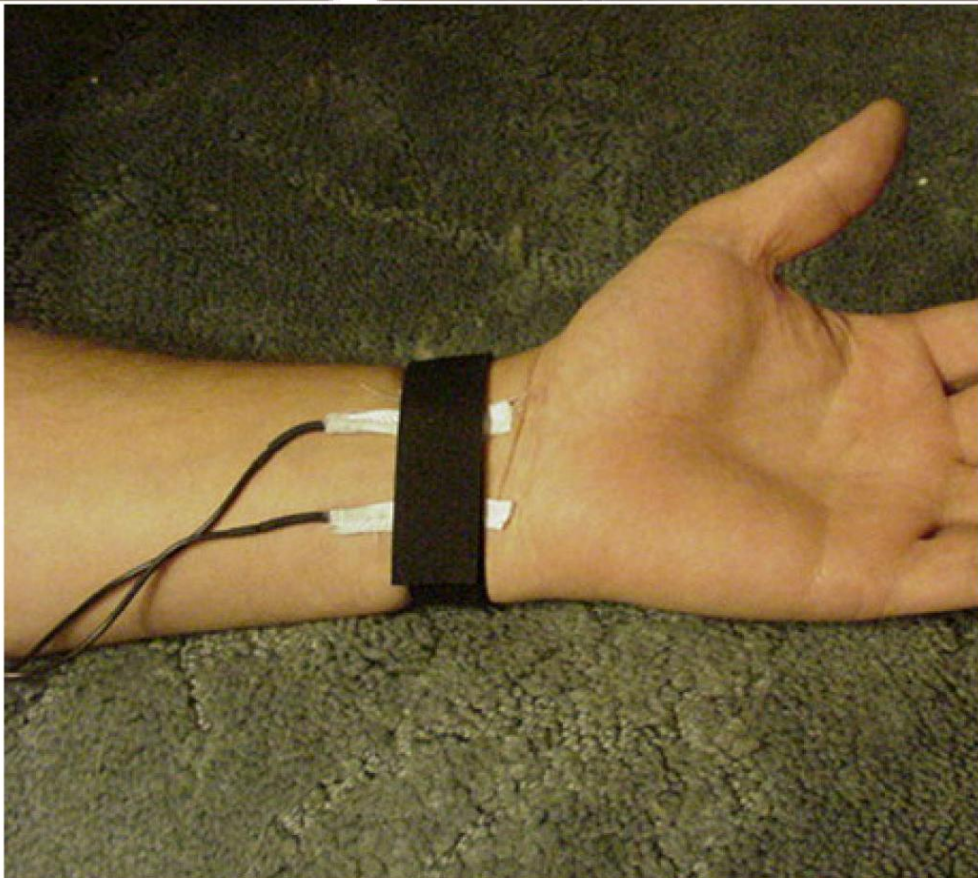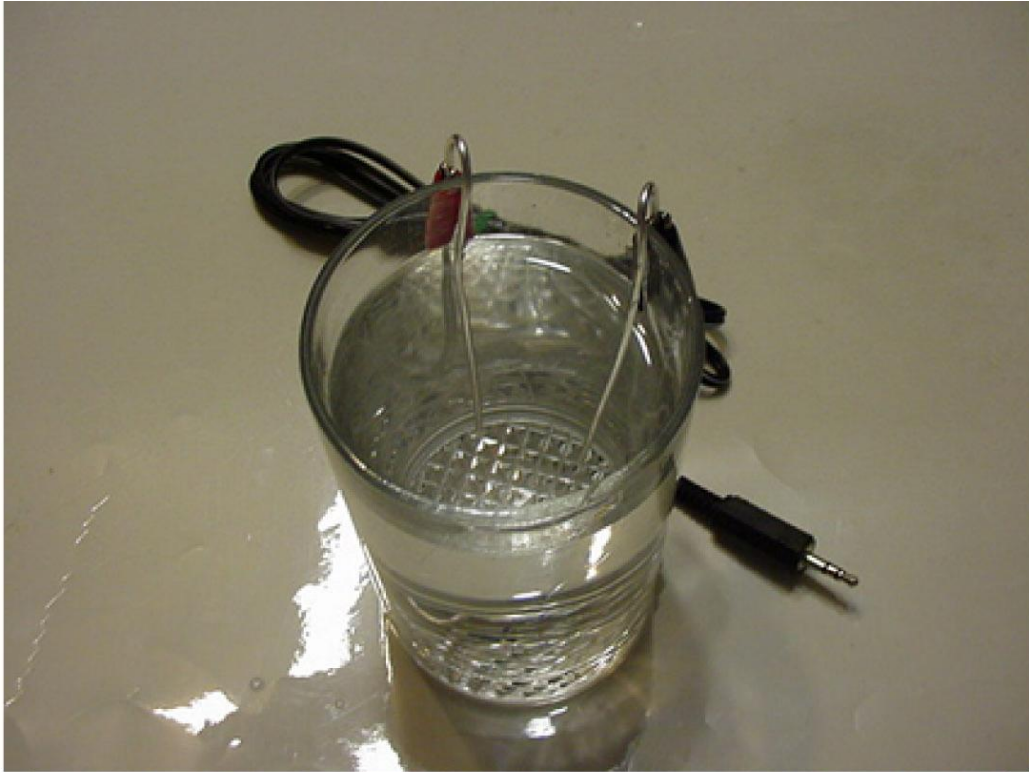

NOTE: BOTH ELECTRODES RUN PARALLEL ALONG THE RADIAL AND ULNAR ARTERIES

